


TABLE TOP TDS METER

Model : Equinox - TDS 101

WITH
ATC

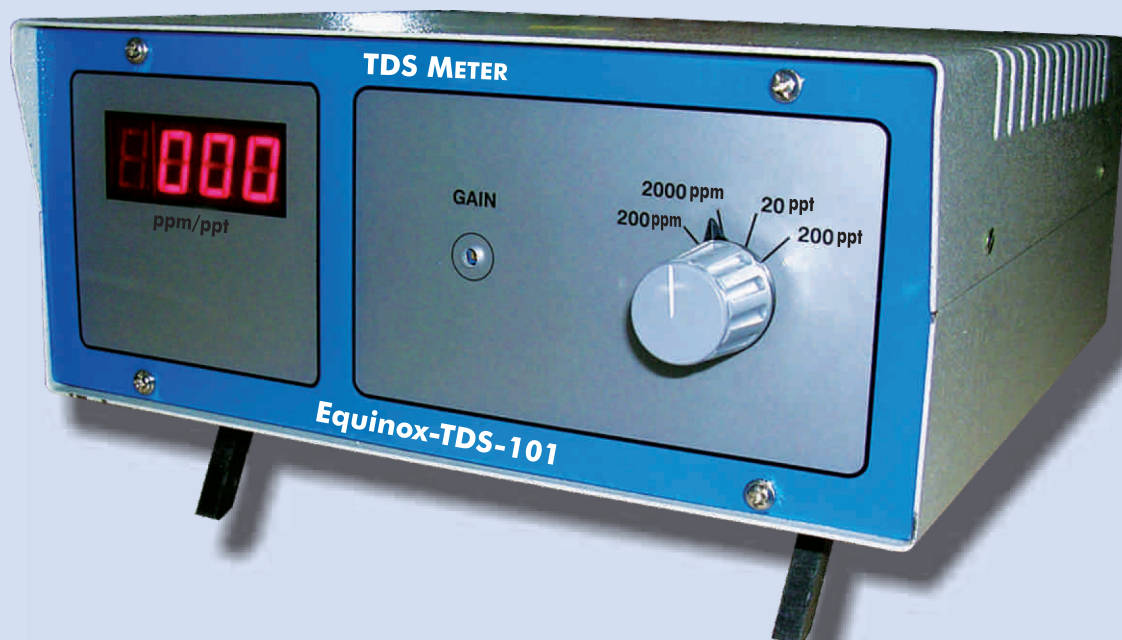

EquinoxTM



HTA INSTRUMENTATION (P) LTD.,

An ISO 9001: 2015 Certified Company & NABL Accredited Calibration Laboratory as per ISO/IEC 17025:2017

Your One Stop For Instrumentation Supply, Automation & Calibration

73, Ramachandra Agrahara, Near T.R. Mills, Chamarajpet, Bangalore - 560018, INDIA.

Phone : 080-26749750, 26759253, 26740681 E-mail : sales@htaipl.com Website : www.htaipl.com



Economy Bench Top TDS Meter

An ergonomically designed lab model TDS meter housed in anti-corrosive enclosure.

1 Features

Bright Red LED	:	Better Visibility even in 'Hard - to See' areas.
Auto Temp Compensation(ATC)	:	Built-In
Accuracy	:	Good accuracy levels to match the Industry Standard.
Calibration	:	1 Point calibration for better stability and accurate readings.
Electrode Holder	:	Provided, for added safety to the electrode.

2 Specifications

Measurement Range	: 0.0 to 199.9 ppm 0 to 1999 ppm 0.0 to 19.99 ppt 0 to 199.9 ppt	Temp. Compensation	: Auto 0 – 60°C
Accuracy	: 1% of F.s. (Excluding Probe Error)	Range Selection	: Manually Using Rotor Switch
Resolution	: 0.1 ppm 1 ppm 0.01 ppt 0.1 ppt	Power Supply	: 230 VAC 1 50 Hz
		Dimensions	: 230 (W)×180(D)×90(H)mm

3 Ordering Information

Order No.	Item
Equinox-TDS 101C	Complete Kit consisting of TDS Meter Conductivity, Electrode of Glass body and of cell constant = 1, Electrode Stand with Clip, One Bottle (200 ml) TDS Buffer Standard of 1000 ppm.
Accessories :	
Equinox-TDS 101	Consists only TDS Meter, Electrode Stand with Clip
Equinox- TDS 101/01E	TDS Electrode of Glass Body and K=1
Equinox- TDS 101/02E	TDS Electrode of Glass Body and K=0.1 (for low TDS Measurement)
Equinox- TDS 101/01S	Electrode Stand with Clip
Equinox- TDS 101/01B	TDS Buffer Standard of 1000 ppm
Equinox- TDS 101/02B	TDS Buffer Standard of 7000 ppm

Authorised Dealer :

Note : We reserve the right to make changes, improvements and modifications to products shown.

TM

EQUINOX